

SPECIFICATION

P/N: CON 3PX28AWG TPV

Customer Reference.

Customer Signed by.

SUZHOU SHS TECHNOLOGY CO.,LTD

苏州尚虹鑫电子科技有限公司

APPROVED	CHECK	DRAWING
 徐 磊 2024.3.12	 徐 磊 2024.3.12	 王思哲 2024.3.12

1. Scope

This specification covers multi micro-coaxial cable for medical equipment.

2. Construction and Material

Item		Unit	Specified Value
Core Number		-	3P
Conductor	AWG Size	-	28
	Material	-	Tinned copper
	Stranding	No./mm	19/0.08
Insulation	Material	-	HDPE
	Color	-	Black/White, Red/Green, Yellow/Blue
	Thickness	mm	0.20
	Diameter	mm	0.80
Twisted		-	See Fig.1
Cabling	Tape	-	AL/PET tape (See Fig.1)
Braid Shield	Material	-	Tinned copper
	Strand	mm	0.08
	Coverage	%	Nom.90
Jacket	Material	-	TPV(Color: Cool Gray)
	Thickness	mm	0.5
	Diameter	mm	4.4±0.2

* Add the filler to make cable round if necessary.

3. Electrical Properties

Item	Unit	Specified Value
Conductor Resistance (@ 20°C)	Ω /km	Max. 210
Insulation resistance (@ 20°C)	MΩ -km	Min. 500
Dielectric Strength ¹⁾	-	To withstand A.C. 500V for 1min
Impedance (@ TDR)	Ω	100±10

1): Applied between each conductor.

4. Package

- 1). Unit length : According to cumtomer requirement.
- 2). Package: Coiled into spool and then packed into carton box

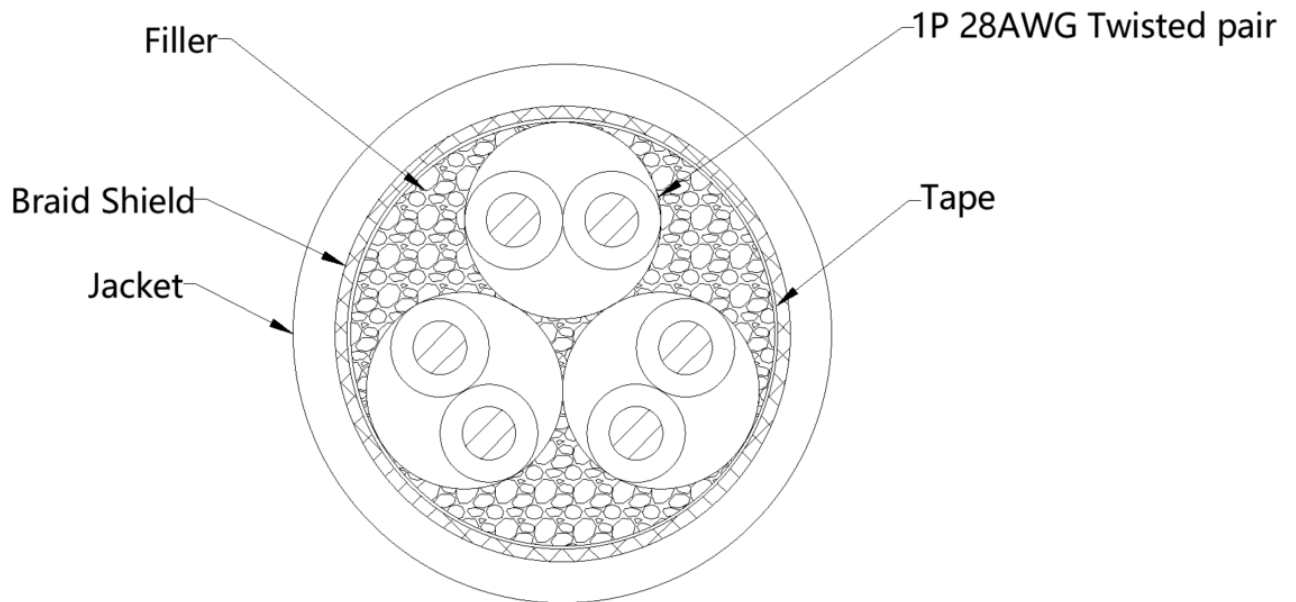


Fig.1 Cross section of cable.

Mail: vincent@shs-tek.com

Add: Room 308, 3rd Floor, Building 2, No.39

Wutaishan, Huqiu District, Suzhou

(From:DE-2001-01 Rev.1)