

SPECIFICATION

P/N: MED 3PX34AWG(VV)

Customer File NO.

Customer Signed by.

SHS TECHNOLOGY CO.,LTD
苏州尚虹鑫电子科技有限公司

APPROVED	CHECK	DRAWING
<div>徐 磊</div> <div>2022.12.1</div>	<div>徐 磊</div> <div>2022.12.1</div>	<div>王思哲</div> <div>2022.12.1</div>

1. Scope

This specification covers mutil wire cable for medical equipment.

2. Construction and Material

Item		Unit	Specified Value
Conductor	Size	AWG	34
	Material	-	Tinned copper
	Stranding	No./mm	7/0.064
Insulation	Material	-	FEP
	Color	-	Blue,Yellow
	Thickness(Nom)	mm	0.052
	Concentricity	%	Min.85
	Diameter	mm	0.30±0.01
Twisted		-	See Fig.1
Shield	Material	-	Tinned copper
	Strand (Nom.)	mm	0.05
	Coverage	%	Nom.90
Jacket(1)	Material	-	Medical TPV (Color: Cool Gray)
	Thickness(Nom)	mm	0.4
	Diameter	mm	1.50±0.15
Cabling		-	See Fig.1
Binder Tape	Material	-	PTFE
Jacket(2)	Material	-	Medical TPV (Color: Cool Gray)
	Thickness(Nom)	mm	0.4
	Diameter	mm	4.2±0.2

3. Electrical Properties

Item	Unit	Specified Value
Conductor Resistance (@ 20°C)	Ω /km	Max. 900
Insulation resistance (@ 20°C)	MΩ -km	Min. 500
Dielectric Strength ¹⁾	-	To withstand A.C. 500V for 1min

1): Applied between each conductor.

4. Package

- 1). Unit length : According customer requirement.
- 2). Package: Coiled and then packed into carton box.

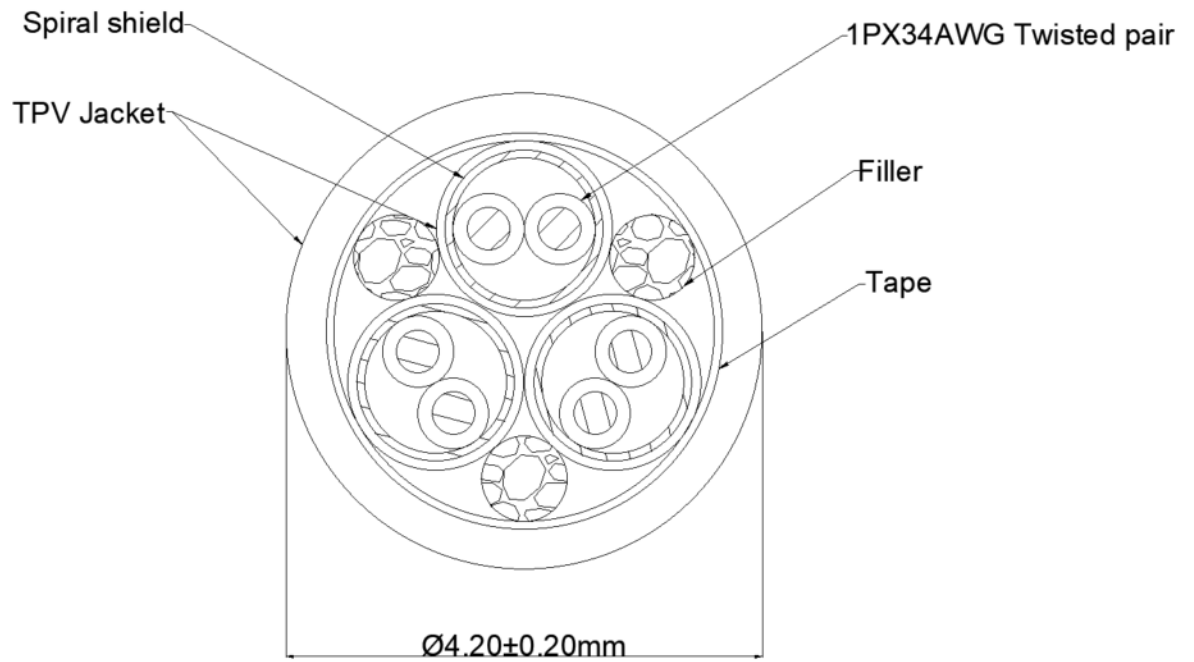


Fig.1 Cross section of cable

